


Printing Paper Contrasts based upon ISO testing methods

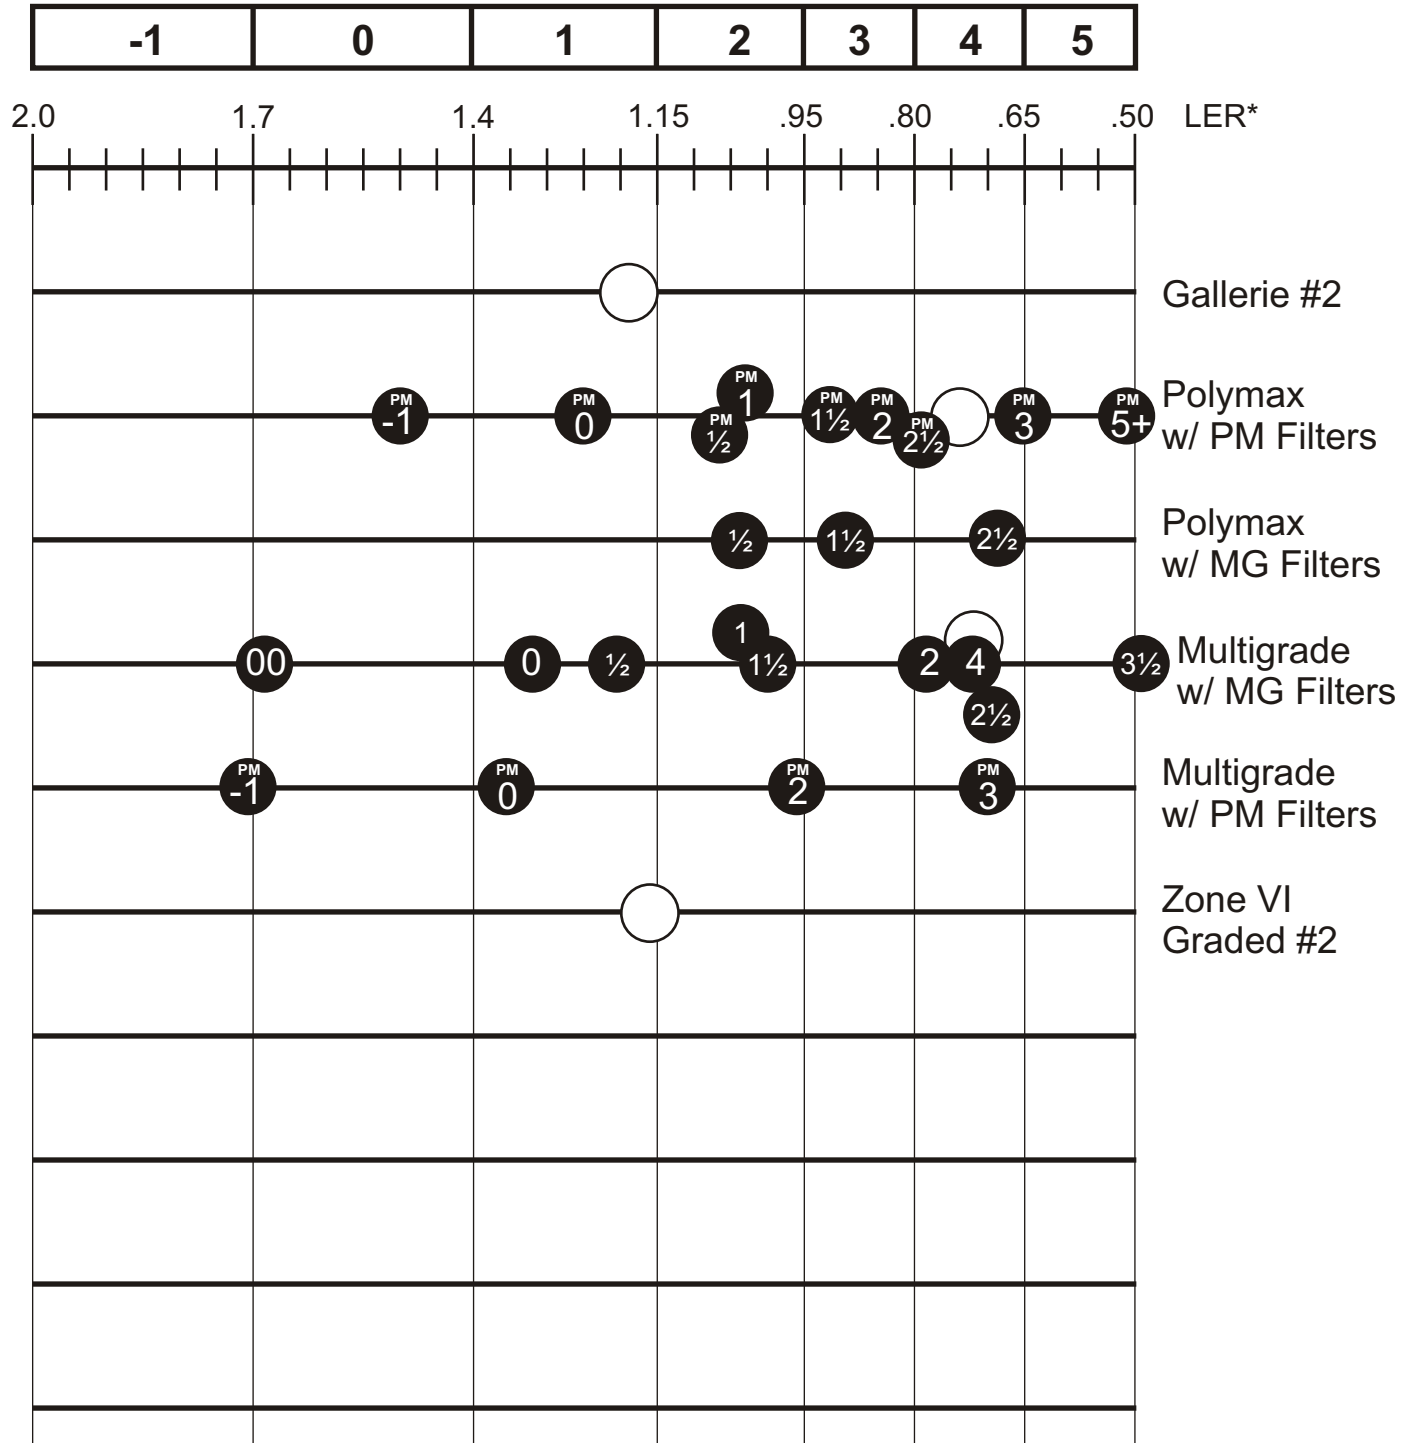

1. All tests done with a Zone VI Cold Light w/ replacement Aristo V54 Lamp

2. My set of Multigrade filters appears to be mislabeled. The #4 filter is clearly more yellow than my #2-1/2. They are out of sequence.

*LER (Light Exposure Range) is measured from a point 0.04 density above paper white and 90% of max black.

*A "PM" above the filter number indicates the use of a Kodak Polymax filter. Otherwise, Multigrade filters were used.



A blank circle indicates that no filter was used under the coldlight illumination